
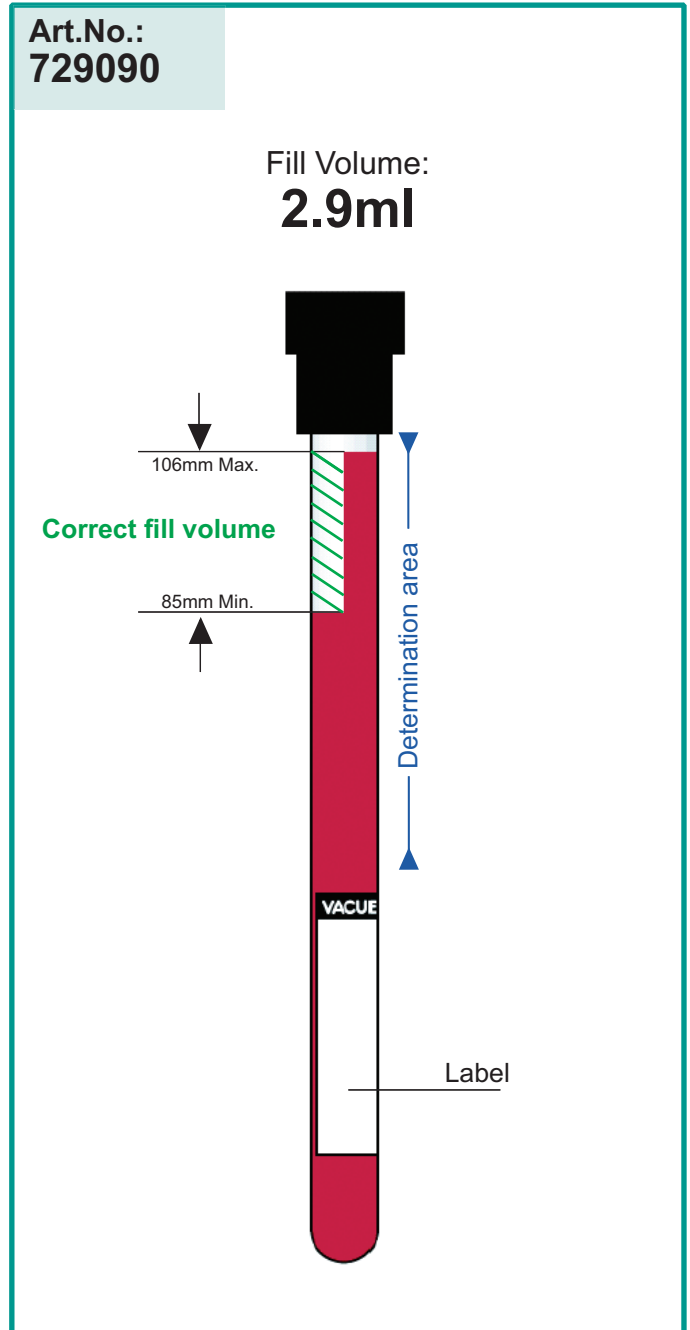


# Greiner Bio-One Customer Information

## VACUETTE® 9/120mm ESR Tubes - 1.6ml, 2.9ml

To check correct fill level of blood sample, please hold the tube against this chart. If the blood level lies between the **"Correct fill volume"** markings on the diagram, then the blood volume is correct.

### Fill volume chart

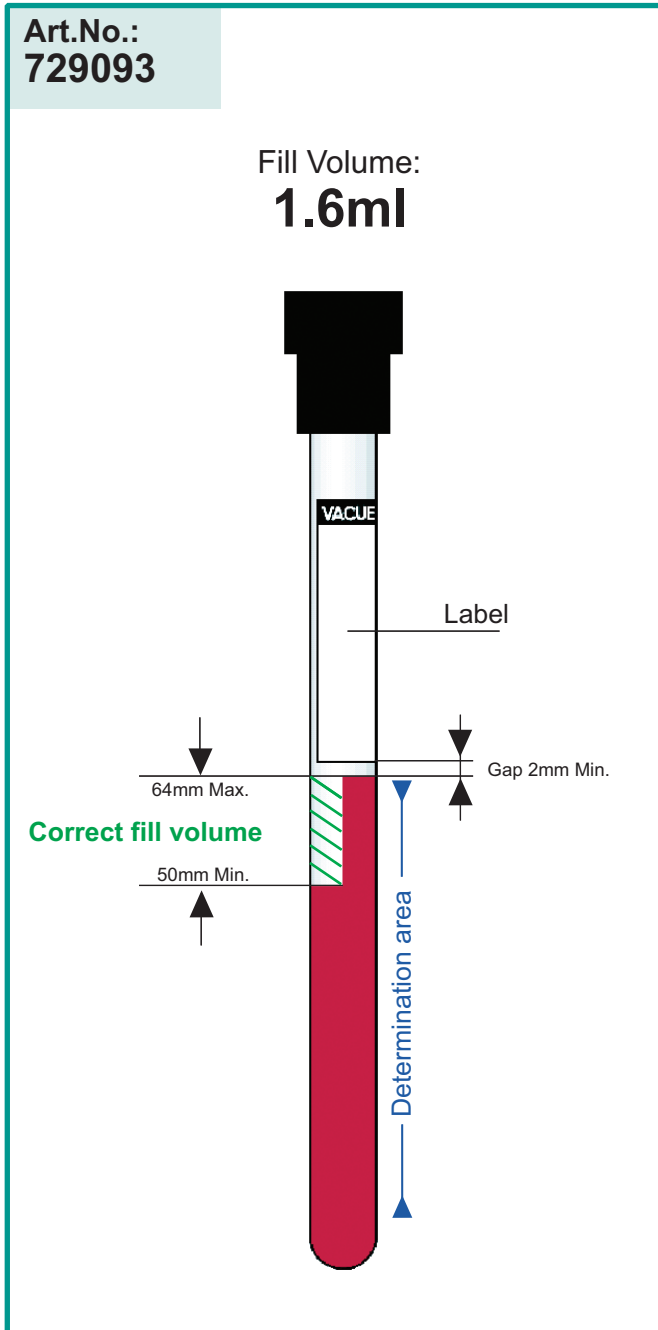

Please do not obstruct the **"Determination area"** with stickers or labels etc. This prevents a correct reading.

Wear gloves during venipuncture and when handling blood collection tubes to minimize exposure hazard.