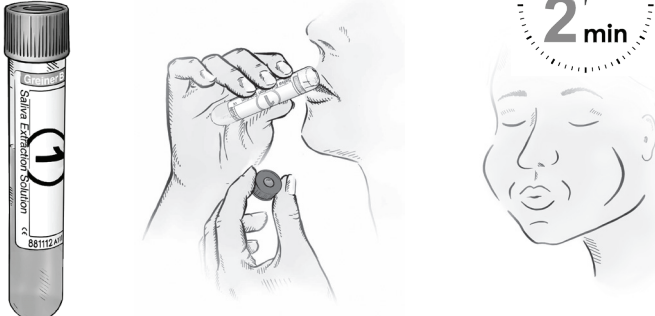


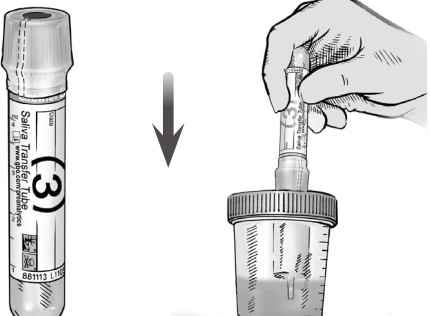


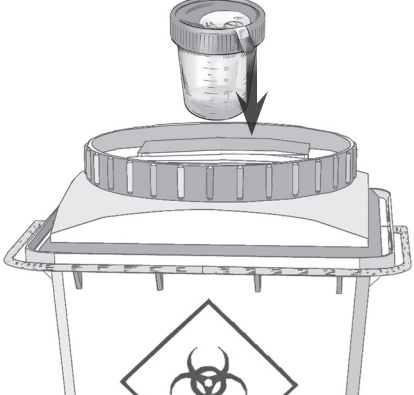



Saliva Collection System

For professional use
Instructions for Use

<p>1</p>  <p>2 min</p>	<p>2</p> 
<p>3</p> 	<p>4</p> 
<p>5</p> 	<p>6</p> 
<p>7</p> 	 <p>Greiner Bio-One GmbH Bad Haller Strasse 32, 4550 Kremsmuenster Austria</p> <p>CE For full instructions please refer to www.gbo.com/preanalytics IFU 980218 and 980244</p>